



(19)

Europäisches Patentamt  
European Patent Office  
Office européen des brevets



(11)

**EP 0 739 603 B1**

(12)

## EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention  
of the grant of the patent:  
22.08.2001 Bulletin 2001/34

(51) Int Cl.<sup>7</sup>: **A61B 17/22, A61B 8/12**

(21) Application number: **96104718.0**

(22) Date of filing: **20.05.1991**

(54) **Intravascular catheter having abrasion head**

Intravaskular-Katheter in Kombination mit einem Schleifkopf

Cathéter intravasculaire muni d'une tête d'outil abrasif

(84) Designated Contracting States:  
**AT BE CH DE DK ES FR GB GR IT LI LU NL SE**

(30) Priority: **21.05.1990 US 528413**

(43) Date of publication of application:  
**30.10.1996 Bulletin 1996/44**

(62) Document number(s) of the earlier application(s) in  
accordance with Art. 76 EPC:  
**91910450.5 / 0 530 296**

(73) Proprietor: **CARDIOVASCULAR IMAGING  
SYSTEMS, INC.**  
**Sunnyvale, CA 94086 (US)**

(72) Inventors:

- **Jang, Yue-Teh**  
**Fremont, California 94539 (US)**
- **Belef, William Martin**  
**San Jose, California 95126 (US)**

(74) Representative: **Nicholls, Michael John**  
**J.A. KEMP & CO.**  
**14, South Square**  
**Gray's Inn**  
**London WC1R 5JJ (GB)**

(56) References cited:

<b>EP-A- 0 347 098</b>	<b>WO-A-89/00023</b>
<b>DE-A- 3 601 453</b>	<b>DE-A- 3 628 684</b>
<b>US-A- 4 850 957</b>	<b>US-A- 4 857 046</b>

**EP 0 739 603 B1**

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

## Description

### BACKGROUND OF THE INVENTION

#### 1. Field of the Invention

[0001] The present invention relates generally to vascular catheters. More particularly, the present invention relates to atherectomy catheters capable of performing abrasion atherectomy, optionally in combination with transluminal imaging.

[0002] The blood vessels of human beings commonly become constricted due to the deposition of fatty substances, e.g., lipoproteins, on the interior of the vessel walls. This condition, known as arteriosclerosis, or atherosclerosis, occurs naturally as a part of the aging process. The condition may also be promoted by such factors as heredity, diet, hypertension, and cigarette smoke. The vascular deposits result in a restriction of blood flow and in serious cases can place a person's health at risk. In acute cases the restriction can result in stroke, hemorrhage, etc. Initially, the fatty deposits are relatively soft; however, over time they become fibrotic and hardened.

[0003] Numerous approaches for reducing and removing intravascular deposits have been proposed. The deposits, called atheromas or atherosclerotic plaques, can be reshaped by dilatation of an inflatable balloon located at the distal end of an angioplasty catheter. Alternatively, atheromas can be removed from the vessel wall by cutting, grinding, or thermal ablation, e.g., via laser angioplasty. Of particular interest to the present invention are atherectomy catheters that remove atheromas from the vessel wall by cutting or grinding.

[0004] In a typical atherectomy operation, a catheter of appropriate diameter is introduced into a patient's vascular system and positioned adjacent the occluding atheroma. The distal end of the catheter is provided with a blade which is brought into contact with the atheroma. The catheter may either be a terminal (front-end) cutting type or a side-cutting type. Side-cutting atherectomy catheters frequently employ an inflatable balloon located opposite the blade to firmly engage the blade with the atheroma.

[0005] However, the above devices have certain deficiencies. In particular, the blades of the cutting element may slice into too much of the occluding material at one time, thereby causing release of large emboli and/or rupture of the vessel wall. Moreover, if the emboli are not promptly captured and removed from the patient's body, they may pass through the vascular system until they become wedged in narrow points of the vascular channels. If an embolus becomes lodged in a critical region of the vascular system, e.g., a coronary artery, the patient's health can be placed seriously at risk.

[0006] The release of large emboli into the vascular system is particularly problematic when front-end cath-

eters are employed. Front-end devices generally employ a cutting element which extends beyond the distal end of a casing for the cutting element. See, for example, U.S. Patent No. 4,857,046. Thus, relatively large particles can be dislodged from the atheroma. Additionally, the dislodged particles generally remain outside the casing of the cutting element, free from entrapment by the catheter. If such particles are not promptly collected they will circulate freely through the vascular system as emboli.

[0007] Side-cutting catheters generally reduce the likelihood that emboli will be released into the vascular system since the housing in which the blades are at least partially contained can passively collect dislodged particles. The collected particles can be removed from the patient's vascular system upon retraction of the catheter. See, U.S. Patent No. 4,794,931. However, many particles can be expected to escape entrapment within the catheter in such a device.

[0008] Several methods have been proposed for remedying the shortcomings identified above. One approach is to modify the impacting head in order to channel dislodged particles into the catheter. See, for example, U.S. Patent No. 4,857,046 which describes an auger-like mechanism for collecting particles. Another approach is to provide an aspiration means for actively removing particles from the vascular system. See, for example, U.S. Patent No. 4,857,045. Still other approaches involve modifying the impacting head to reduce the size of the dislodged particles in an effort to minimize the risk to the patient presented by large emboli. See, for example, Fig. 4 of U.S. Patent No. 4,857,045. None of the approaches proposed for reducing the size of particles and for capturing and withdrawing the particles provides a satisfactory solution for these problems.

[0009] For these reasons it is desirable to provide catheters that grind atheromas into very small debris particles. Also, it is desirable to remove those particles via catheters provided with flushing and aspiration means for removing the particles. Such devices are expected to significantly reduce the potential for release of large emboli. Additionally, it is desired to provide a means for transluminally imaging the site of atherectomy in order to determine the location and extent of removal of the undesired tissue.

#### 2. Description of the Background Art

[0010] U.S. Patent Nos. 4,857,046, 4,857,045, 4,842,578, 4,747,821, 4,631,052, and 4,795,438 all describe front-end intravascular catheter devices. None of the references describe devices that grind away atherosclerotic plaques via an impacting head that is substantially contained within a housing. Nor do the devices utilize an inflatable balloon means to aid engagement of the impacting head with the undesired tissue. US-A-4 794 931 describes a catheter having a rotary impacting head which removes sclerotic material through a side

window provided in a housing. An opposing balloon is provided to assist placement of the head adjacent the undesired material. US-A-4 794 928, 4 465 072 and 3 889 657 relate to catheter designs intended to scrape blood vessels and other body lumens.

[0011] Various techniques for transluminal imaging of the diseased region of a vessel wall have been proposed, including endoscopic and ultrasonic imaging techniques. See, for example, US-A-4 794 931 which describes an ultrasonic transducer attached to the hub of a rotary head. See, also, US-A-5 029 588 which describes a laser catheter having transluminal imaging capability, and US-A-5 117 831 which describes a combined balloon angioplasty/imaging catheter.

[0012] A catheter comprising the features of the preamble of Independent Claim 1 is known from US-A-4 850 957.

[0013] According to the present invention, there is provided an intravascular catheter for removing stenotic material from a patient's vascular system, said catheter comprising:

- an elongate catheter body having proximal and distal ends;
- a housing attached to the distal end of the catheter body, said housing having an open interior and an aperture therethrough;
- a rotatable member substantially within the housing;
- means for rotating the rotatable member; and
- means within the catheter body for withdrawing abraded material from within the housing; characterised in that the rotatable member has a substantially cylindrical outer abrasive surface for abrading stenotic material that penetrates the aperture so that abraded material collects within the housing.

[0014] A preferred embodiment of the invention has an aspirating means connected to the interior of the housing via an axial lumen provided in the catheter body. Abraded stenotic material is thereby aspirated from the patient's body. Additionally, grooves (or channels) may be provided axially or helically along the exterior of the abrasive head or along the interior wall of the housing. Such grooves assist in transport of abraded material from distal the head to points proximal the head. A flushing means located external the patient's body may also be employed to augment removal of material from within the catheter housing.

[0015] Another preferred embodiment has a transluminal imaging means affixed to the head for abrading the stenotic material. Preferably, the transluminal imaging means is afforded by an ultrasonic transducer.

[0016] A further preferred embodiment of the invention employs at least one inflatable balloon attached to the housing. Inflation of the balloon(s) assists in contacting the stenotic material with the abrasive head when the housing aperture is provided in a side wall of the

housing.

[0017] Placement of the rotary member within the housing helps ensure that dislodged particles collect inside the housing. Exemplary surfaces of the rotatable member are comprised of diamond powder and fused silica, tungsten carbide, aluminum oxide, boron carbide, and the like. The rotatable member can have an axial lumen through which a guidewire may be passed. Imaging of the site of occlusion may be provided by an ultrasonic transducer affixed to the rotatable member.

[0018] The present invention thereby affords superior grinding devices for removing stenotic material from a patient's vascular system.

[0019] The invention will be further described by way of example with reference to the accompanying drawings, in which:-

[0020] Fig. 1 is a detail view of the distal region of a front-end catheter constructed in accordance with the principles of the present invention.

[0021] Fig. 2 is a detail view of the distal region of a side-on catheter constructed in accordance with the principles of the present invention.

[0022] Fig. 3 is a cross-sectional view taken along line 3-3 of Fig. 1.

[0023] Fig. 4 is a cross-sectional view taken along line 4-4 of Fig. 2.

[0024] Fig. 5 is a cross-sectional view of an alternative housing embodiment constructed in accordance with the principles of the present invention.

[0025] Figs. 6A-D present perspective and end-on views of exemplary front-end abrasive heads constructed according to the principles of the present invention.

[0026] Figs. 7A-E present perspective views of exemplary side-on abrasive heads constructed according to the principles of the present invention.

[0027] Figs. 8A-C show cross-sectional views of alternative catheter bodies constructed according to the principles of the present invention (Fig. 8A is taken along line 8-8 of Fig. 2).

[0028] Fig. 9 is a detail view of a side-on catheter having an alternative design for provision of means for withdrawing abraded material.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0029] According to the present invention, intravascular catheters will include an elongated catheter body having distal and proximal ends. The catheter body will include an abrasive head for abrading stenotic material at the distal end of the catheter body. Preferably, the abrasive head will be provided by an abrasive rotatable member contained substantially within the housing. The housing will be provided with an aperture to permit intrusion of the stenotic material into the housing cavity. At least part of the periphery of the aperture is expected to contact target stenotic material during operation of the abrasive head, thereby assisting in containment of

particles released by the grinding process. Also, means for withdrawing abraded material from within the housing to a point external the patient is provided. Preferably, an aspirating means in communication with the interior of the housing via a axial lumen in the catheter body will be employed as the means for withdrawing abraded material.

[0030] In a preferred embodiment, the aperture of the housing located at the distal end of the catheter will be provided in a side wall of the housing. One or more inflatable balloons will be optionally provided opposite the aperture to permit anchoring the distal end of the catheter adjacent a target stenosis.

[0031] The stenotic material that can be abraded by the present devices includes all naturally occurring occlusions of vascular walls, e.g., atherosclerotic plaques, lipoprotein deposits, blood clots, hemorrhaged tissues, etc.

[0032] Catheters constructed according to the present invention also may include a transluminal imaging means affixed to the abrasive head. Such imaging means preferably will be provided by ultrasonic transducers. Suitable transducers are described in U.S. Patent No. 4,794,931.

#### A. Catheter Bodies.

[0033] The vascular catheters of the present invention will comprise a catheter body having distal and proximal ends. The catheter body will be flexible to permit its passage through the vascular system of a patient. Preferably the catheter body will be comprised of a flexible transparent thermoplastic that affords ready visual inspection for air bubbles inside the catheter body. The catheter body will preferably have a smooth tubular shape; however, the catheter body may have a ridged structure, particularly when it is desired to provide a lumen, e.g., a guidewire lumen, along the longitudinal axis of the catheter.

[0034] The catheter selected will have an outer diameter small enough to permit positioning adjacent the diseased region of the vessel wall. Typically, the outer diameter of catheters employed will be in the range from about 1 mm to 4 mm, usually being about 2.5 mm for peripheral arteries of adult humans and about 1.7 mm for coronary arteries. Catheters employed will typically have a length ranging from about 60 cm to 150 cm.

[0035] Referring now to Fig. 1, a front-end type vascular catheter constructed in accordance with the principles of the present invention includes an elongated catheter body 110 having distal 112 and proximal 114 ends. Catheter body 110 is connected at its proximal end 114 to a manifold (not shown) via manifold connector 116. Such manifold connector includes internally-threaded means for connecting catheter body 110 to the manifold and is well known to those skilled in the art. The distal end of the catheter may be adapted to accept a moveable guidewire, described more fully herein be-

low.

[0036] Catheter body 110 is comprised of a flexible plastic tube 118 having an outer diameter suitable for insertion into the patient's target vessel. Plastic tube 118 is preferably comprised of a transparent thermoplastic to permit observation of air bubbles internal the tube. Tube 118 is flexible and includes at least one lumen extending from the distal end 112 to the proximal end 114 thereof. Additional lumens may be included as needed. The utility of such lumens is discussed in more detail below.

[0037] Catheter body 110 is provided at its distal end with housing 120. Housing 120 preferably is constructed from stainless steel and is attached to plastic tube 118 using conventional methods. See, for example, U.S. patent application Serial Nos. 732,691 and 834,893 (now U.S. Patent No. 4,794,931). In front-end type catheters an aperture 122 is provided in the distal tip of housing 120 to permit penetration of target stenotic material into housing cavity 124. Housing cavity 124 contains all void space within housing 120 and is defined at its distal end by the periphery of aperture 122 and at its proximal end by flexible tube 118. Abrasive head 126 is provided internal housing 120 and is capable of moving axially or rotationally within housing cavity 124. A cross-section of housing 120 along line 3-3 is presented in Fig. 3, which is discussed herein below.

[0038] Fig. 2 shows the distal region of a side-on catheter constructed in accordance with the principles of the present invention. Catheter body 210 has essentially the same dimensions and is constructed from essentially the same materials as front-end catheter bodies described above. Catheter body 210 has distal end 212 and proximal end 214 thereof. Proximal end 214 is connected to a conventional manifold connector (not shown). A conventional fixed guidewire 215, described more fully herein below, is secured to distal end 212. Flexible tube 216 is comprised of the same materials and has essentially the same configurations allowed for the corresponding tube for front-end catheters described above.

[0039] Flexible tube 216 is attached to housing 218 in conventional manner. Housing 218 is typically comprised of stainless steel and has a cylindrical shape. A portion of the sidewall of housing 218 is removed to present aperture 220, through which stenotic material may penetrate into housing cavity 222. The distal tip of housing 218 may optionally be provided with an orifice through which a guidewire can pass.

[0040] In a preferred embodiment, at least one inflatable balloon is provided external the housing so as to press the side of the housing having the aperture against the target stenotic material. For example, as shown in Fig. 2, inflatable balloon 224 is provided opposite aperture 220 and external to housing 218. Balloon 224 is securely attached to housing 218, e.g., via a suitable adhesive. The proximal extremity of balloon 224 is preferably bonded to flexible tube 216 via a heat-shrink-

able material. Balloon 224 can be inflated by passing an inflation medium through an inflation orifice 226 provided proximate the proximal extremity of balloon 224. Other aspects of the inflatable balloon feature of side-on catheters are presented in U.S. Patent No. 4,794,931.

[0041] Fig. 4 presents a cross-sectional view of the side-on catheter of Fig. 2 taken along line 4-4 thereof. Thus, housing 218 defines housing cavity 224 and is provided with aperture 220 with balloon 222 provided opposite aperture 220.

#### B. Abrasive Heads.

[0042] In the present invention, an abrasive head is provided at the distal end of the catheter body. The head is contained substantially within the housing located at the distal end of the catheter body. It is contemplated that a portion of the abrasive head may extend from within the housing to a point beyond the aperture provided in the housing; however, the entirety of the head will be contained within the housing sufficiently to ensure that dislodged stenotic material will be substantially contained within the housing.

[0043] The abrasive head may be comprised of a unitary abrasive material or may be a composite of a support material and an abrasive surface material affixed to the support. When an abrasive surface material is employed it may be adhesively bonded to the support by methods well known to those skilled in the art. Preferred abrasive materials comprising the surface of the abrasive head include fused silica, diamond powder, tungsten carbide, aluminum oxide, boron carbide, and other ceramic materials. Suitable abrasive materials are available commercially from Norton Company, Worcester, Massachusetts.

[0044] When a composite abrasive surface and solid support is employed as the abrasive head of the present invention, a suitable support material must be identified. Generally, a suitable support will be any solid material that bonds effectively to the abrasive surface material with an adhesive. The support further must withstand the inertial and impact forces experienced during operation of the abrasive head.

[0045] A preferred support material is stainless steel. Also, the support preferably has an axial lumen to allow passage of a guidewire therethrough.

[0046] Typically, the abrasive head is attached to a drive means via a coupling provided at its proximal end. The drive means will extend axially through a lumen provided in the catheter body to a point external the patient's body. The drive means is connected to a drive motor which provides the power for driving the abrasive head. The drive means preferably includes an internal lumen which permits passage of a guidewire if desired.

[0047] Operation of the drive means is such that one revolution of the drive means causes one revolution of the abrasive head. During operation, the drive means will usually make 200-100,000 revolutions per minute.

Also, translation of the drive means relative to the catheter body causes a translation of the abrasive head relative to the catheter body. Translation and rotation of the abrasive head via the drive means is afforded so as to permit the head to contact stenotic material that penetrates the aperture of the housing. The construction and operation of drive means suitable for use in the present invention is further described in U.S. Patent No. 4,794,931.

#### 1. Front-end Catheters.

[0048] When the catheter is of the front-end type, the abrasive head contained substantially within the housing will have an abrasive surface at the distal-most end of the head. Abrasive surfaces may also be provided elsewhere on the head. The proximal-most end of the head is in communication with a means for driving the head, e.g., a drive cable or a compressed fluid means.

[0049] Fig. 3 presents a cross-sectional view of the head and housing of the front-end type catheter shown in Fig. 1. Thus, an abrasive rotatable member 126 is provided internal housing 120 and is positioned so as to permit engaging rotatable member 124 with any stenotic material that penetrates the aperture 122 in the distal end 112 of housing 120. The rotatable member 126 need not be wholly contained within housing 120, i.e., the most distal region of the rotatable member may extend through aperture 122; however, rotatable member 126 must remain sufficiently within housing 120 such that the abrading surface of the rotatable member remains substantially within housing cavity 124 defined at its most distal end by aperture 122.

[0050] Grooves (or channels) are optionally provided axially along the exterior wall of the abrasive head to assist passage of dislodged material from the distal-most end of the housing to a point proximal the head. For example, Fig. 3 shows an abrasive rotatable member 126 provided within housing 120. The outer periphery of rotatable member 126 is provided with two grooves 128. An abrasive head having grooves may have only one groove or may have a plurality of grooves. Preferably, the grooves will be spaced equally about the periphery of the head; however, such equal spacing is not necessary. Abrasive rotatable member 126 is also provided with lumen 130 which permits passage of a guidewire therethrough and may also assist in the withdrawal of released particles from the distal region of the head.

[0051] Grooves may additionally or optionally be provided axially along the interior surface of the housing. For example, Fig. 5 shows a cross-sectional view of an exemplary housing 510 having four equally spaced grooves 512 along the interior surface of housing 510. The same or similar designs having housings provided with interior grooves are also suitable for side-on catheters. The grooves or channels will usually be oriented in a generally axial direction but it will also be possible to dispose the grooves helically so long as they provide

or allow for proximal translation of the abraded material passed the head.

[0052] Referring now to Figs. 6A-D some exemplary front-end abrasive heads in accordance with the principles of the present invention are presented. Both side views and end-on views are presented. Other abrasive heads consistent with the principles of the present invention will be apparent to those skilled in the art.

[0053] Fig. 6A shows head 610 having a cylindrical body 612 capped at its distal end by a rounded, e.g., hemispherical, abrasive surface 614. Cylindrical body 612 is provided with four periodic grooves 616 which permit withdrawing abraded material from a region distal the head to a region proximal the head. An end-on view of the head shows the abrasive surface 618 periodically grooved around its periphery. Drive means 620 is attached to the proximal end of head 610 and extends proximally to a point external the patient's body.

[0054] Fig. 6B shows an alternative head design in which head 630 has a cylindrical body and a concave depression 632 provided at its distal end. An end-on view of head 630 shows an abrasive surface 634 having a circular periphery and an orifice 636 provided central to the surface through which a guidewire (not shown) may pass. Preferably, when a guidewire is employed, the wire will pass through the interior of head 630 via orifice 636 and will extend through an axial lumen provided interior drive means 620. The concave design of this and other such heads is expected to further assist in containing particles released upon grinding.

[0055] Fig. 6C shows another embodiment of an abrasive rotatable member of the present invention. Rotatable member 640 has a cylindrical body in which periodic grooves 642 are axially provided. The distal end 644 of rotatable member 640 has a recessed abrasive surface 646. The periphery of abrasive surface 646 is grooved at points corresponding to periodic grooves 642.

[0056] Fig. 6D presents a further embodiment of an abrasive rotatable member according to the principles of the present invention. Rotatable head 650 has a substantially cylindrical body provided with periodic grooves 652 running axially along its surface. The distal end 654 of head 650 has a substantially planar abrasive surface 656 attached thereto. The periphery of surface 656 has indentations accommodating periodic grooves 652. The center of surface 656 is provided with orifice 658 through which a guidewire may pass. Imaging transducer 660, e.g., an ultrasonic transducer, is affixed to surface 656.

## 2. Side-on Catheters.

[0057] The abrasive heads of the present invention that are suitable for use in side-on catheters are comprised of the same or similar materials and are constructed analogously to the heads described above for front-end catheters. However, the side-on catheters of the present invention can be contrasted from front-end designs in that side-on designs allow use of a pull-type

abrasive head, in which an abrasive surface is provided on the proximal end of the head.

[0058] Referring now to Fig. 2, housing 218 is provided with aperture 220. Preferably, aperture 220 is provided as an elongated slit in housing 218. Housing 218 further defines internal region 224 in which an abrasive head (not shown) will be provided. Moreover, internal region 224 will be at least partially occupied by target stenotic material and debris during operation of the device. Inflatable balloon 222 is provided opposite aperture 220 and external to housing 218. During inflation of inflatable balloon 222, an inflation medium is passed into balloon interior 228 provided between balloon 222 and housing 218. Likewise, deflation of balloon 222 occurs upon removal of inflation medium from the balloon interior 228. Inflation and deflation operations are described more fully below.

[0059] Referring now to Figs. 7A-E, exemplary side-on abrasive heads are presented. Thus, in Fig. 7A, abrasive head 710 is comprised of a cylindrical region 712 and a conical region 714 distal to the cylindrical region. Conical region 714 is provided with an abrasive surface, which preferably extends over the entirety of the conical region. The cylindrical region 712 of head 710 is provided with periodic grooves 716 which allow passage of particles and fluid from distal head 710 to proximal head 710. Orifice 718 is provided in the distal tip of conical region 714 to allow passage of a guidewire. Drive means 720 is attached proximally to head 710 to allow translation and/or rotation of head 710 to contact the abrasive surface of the head against stenotic material.

[0060] Fig. 7B depicts another preferred embodiment of an abrasive head suitable for removing stenotic material via a side-on atherectomy catheter. Thus, the head is comprised of cylindrical region 722 proximally attached to conical region 724. Conical region 724 has an abrasive surface, preferably extending over the entirety of region 724. The proximal-most tip of conical region 724 is attached to drive means 720.

[0061] Fig. 7C presents a further preferred embodiment of a side-on abrasive head. Thus, the head comprises cylindrical region 730 attached at its distal and proximal ends to conical regions 732 and 734, respectively. Both regions 732 and 734 are provided with abrasive surfaces. Cylindrical region 730 is provided with periodic grooves 736 and is further provided with transducer 738. The proximal terminus of region 734 is attached to drive means 720.

[0062] Fig. 7D shows a further preferred embodiment of a suitable side-on abrasive head in which an abrasive surface is provided over at least part of cylindrical region 740. Cylindrical region 740 is further provided with periodic grooves 742 as described above. Transducer 744 is provided in a recess on the surface of region 740.

[0063] In Fig. 7E, the abrasive head is comprised of two conjoined abrasive regions. Thus, cylindrical region 750 is joined to conical region 752 provided distally to cylindrical region 750. Groove 754 is provided axially

along cylindrical region 750.

[0064] Clearly, other designs of abrasive heads are contemplated in accordance with the principles of the present invention. Such designs will be readily apparent to one skilled in the art.

### C. Means for Withdrawing Material.

[0065] A means for withdrawing dislodged stenotic material from within the housing for the abrasive head is provided internal the catheter. Such provision permits removal of debris generated by the grinding process soon after it is produced, thereby greatly reducing the likelihood of emboli being released into the vascular system. Provision of such withdrawing means integrally to the catheter body also precludes the need for a means for withdrawing debris that is independent of the catheter.

[0066] Generally, the means for withdrawing abraded material will be the same for front-end or side-on catheters. However, some distinctions between front-end and side-on embodiments with respect to provision of the withdrawing means are envisioned and are described below.

[0067] Preferably, the means for withdrawing abraded stenotic material will principally employ an aspiration means in communication with the housing chamber internal the housing. Such means will ensure a negative pressure is maintained within the housing chamber relative to the surrounding vascular system, thereby minimizing the chance of emboli release from the housing chamber. The location selected for the aspiration opening within the housing is noncritical; however, it will preferably be distal the housing chamber and relatively near the aperture of the housing in order to minimize the time abraded material is retained within the housing.

[0068] Additionally, the means for withdrawing abraded material from the housing chamber may include a flushing means in communication with the chamber. The flushing means will employ a biocompatible flushing medium. Suitable flushing media are well-known to those skilled in the art and include saline and electrolyte solutions.

[0069] Care must be taken to ensure that the introduction of flushing media into the region internal the housing does not significantly promote release of emboli into the vascular system. Since release of emboli from within the housing will most likely occur through the aperture of the housing, flushing media will preferably be introduced into the housing chamber at a point within the housing that is as distant from the aperture as possible.

[0070] Further, it is preferred that the point selected within the housing for introducing the flushing medium will be chosen so as to maximize the coverage, or "sweep," of flushing media throughout the interior of the housing. Such provision will favor separation of the introduction point of the flushing medium from the point

selected for the aspiration opening.

[0071] An exemplary preferred embodiment of the above-described means for withdrawing abraded material is presented in Fig. 9. Thus, the distal region 910 of a side-on catheter has flexible tube 912 attached to housing 914. Housing 914 is provided with an aperture 916 and with inflatable balloon 918 located opposite the aperture. Abrasive head 920 is located in housing chamber 922 internal housing 914 and is connected at its proximal end to drive means 924. Drive means 924 extends proximally through a lumen provided in flexible tube 912. A moveable guidewire will pass through a lumen provided internal in drive means 924. The guidewire will extend through the entire length of catheter 910 and will extend proximally and distally therefrom, as described more fully herein below.

[0072] An inflation medium will be introduced into catheter 910 via inflation lumen 926 provided in flexible tube 912. The inflation medium will pass through orifice 928 provided at the proximal extremity of housing 914 and into inflation region 930 located between balloon 918 and housing 914.

[0073] Flexible tube 912 is further provided with aspiration lumen 932 which extends axially therethrough and terminates distally in aspiration orifice 934 located at the interface between housing chamber 922 and flexible tube 912. Flexible tube 912 is further provided axially with flushing lumen 936 which extends distally to the proximal end of flushing tube 938 provided within housing chamber 922. Flushing tube 938 and flushing lumen 936 are met so as to prevent leakage of flushing medium there between. Flushing medium will pass through a lumen provided in flushing tube 938 until reaching flushing orifice 940 located distally in housing chamber 922.

[0074] Other embodiments incorporating the means for withdrawing abraded material from within the housing will be apparent to the skilled practitioner in view of the principles of the present invention.

### D. Imaging Transducers.

[0075] Frequently, an imaging means will be employed to afford a transluminal image of a diseased region of the patient's vascular system. Preferably, an ultrasonic transducer will be used to generate the imaging medium. A preferred transducer, its associated circuitry, and a preferred mode of operation are described in U. S. Patent No. 4,794,931.

[0076] For example, Fig. 7D shows a cylindrical abrasive head suitable for use in a side-on catheter device according to the principles of the present invention. Transducer 744 is attached to the exterior of abrasive rotatable member 740. The transducer 744 will preferably be positioned in a recess provided in the surface of member 740. The recess will be sufficient to ensure that transducer 744 does not interfere with abrasion of atheromatous material. Typically, transducer means 744 will be circular in shape and will have an outer diameter of

0.635-2.54 mm (0.025-0.100 inches).

#### E. Guidewires.

[0077] The catheters of the present invention will usually be used in conjunction with a guidewire. The guidewire will be either a fixed or moveable type. When a fixed guidewire is used, the distal end of the catheter will be secured to the guidewire. The guidewire will help to identify the vascular channel through which the catheter will pass, thereby assisting in placement of the distal end of the catheter adjacent stenotic material.

[0078] When a moveable guidewire is employed the guidewire will be first inserted into a patient's vascular system. The guidewire will pass to the target stenotic material. The distal end of the catheter will be guided to the site of occlusion by the guidewire. Usually, the guidewire will pass through an orifice provided in the distal tip of the catheter and will pass through the interior of the housing, typically via a lumen provided in the abrasive head. The guidewire will extend proximally through a lumen provided for such purpose in the catheter until the guidewire exits the patient's body.

[0079] Figs. 8A-C present cross-sectional views of exemplary catheter bodies incorporating a lumen for passage of a guidewire therethrough. For example, Fig. 8A shows flexible tube 810 of the catheter body provided with lumen 812. Lumen 812 affords passage of drive means 814 which is itself provided with guidewire lumen 816. Flexible tube 810 is further provided with lumens 818, 820, and 822 which provide, respectively, means for aspirating dislodged material, means for flushing, and means for inflating an inflatable balloon.

[0080] A cross-sectional view of a catheter body having an alternative design, is shown in Fig. 8B. Thus, flexible tube 830 is provided with lumen 832 which accommodates drive means 834. As shown, drive means 834 need not have an axial lumen therethrough since the guidewire is passed through a separate lumen in flexible tube 830. Flexible tube 830 is further provided with lumens 836, 838, and 840 which allow, respectively, passage of a guidewire, aspirating means, and flushing means. Such a design is preferred when an inflatable balloon need not be present, e.g., when a front-end type catheter is employed.

[0081] Fig. 8C shows a cross-sectional view of another preferred embodiment, in which the guidewire passes through a lumen provided in the flexible tube of the catheter body. Thus, flexible tube 850 is provided with an axial lumen 852 which accepts drive means 854. Flexible tube 850 is further provided with lumens 856, 858, 860, and 862 which permit, respectively, passage of a guidewire, aspiration means, flushing means, and inflation means.

[0082] Other lumen patterns are consistent with the principles of the present invention and will be apparent to one skilled in the art. The inner diameter of a lumen provided for a guidewire will vary according to the diam-

eter of the catheter but will typically be 0.254-0.508 mm (0.010-0.020 inches) for smaller catheters and 0.835-1.016 mm (0.025-0.040 inches) for larger catheters.

#### F. Method of Use.

[0083] Preferably, the distal end of the catheter and its abrasive head will be positioned adjacent target stenotic material with aid of X-ray fluoroscopy which readily identifies a catheter's location internal the patient. Such methods are well-known to those skilled in the art.

[0084] When a side-on catheter is employed, an inflation balloon is preferably located opposite the target deposit to cause the material to penetrate the aperture of the housing containing the abrasive head. The abrasive surface of the head will grind against the stenotic material through a combination of rotational and translational motion until the material is effectively removed from the vessel wall. Debris generated by the grinding process will be vacuum aspirated via an aspirating means external the patient. Preferably, a flushing medium is provided to assist withdrawal of the particles. The site of occlusion is inspected either concurrent with or subsequent to the grinding process to determine the extent of removal, preferably by means of an ultrasonic transducer located on the surface of the abrasive head. The above series of steps can be repeated at a different site of occlusion in the same manner.

[0085] Although the foregoing invention has been described in detail for purposes of clarity and understanding, it will be obvious that certain modifications may be practiced within the scope of the appended claims. For example, catheters constructed according to the principles of the present invention may be equipped with two balloon members to better anchor the catheter in the vascular system. Also, when two balloons are provided, they may be offset from directly opposite the aperture of the housing, thereby allowing removal of a portion of the housing directly opposite the aperture. Such a configuration will allow imaging of the vessel wall directly opposite target stenoses.

#### G. Claims

1. An intravascular catheter for removing stenotic material from a patient's vascular system, said catheter comprising:

an elongate catheter body (110, 210, 910) having proximal and distal ends (114, 214; 112, 212);

a housing (120, 218, 914) attached to the distal end (112, 212) of the catheter body (110, 210, 910), said housing (120, 218, 914) having an open interior and an aperture (122, 220, 916) therethrough;



- a rotatable member (126, 920) substantially within the housing (120, 218, 914); means (924) for rotating the rotatable member (126, 920); and means (932-940) within the catheter body (110, 210, 910) for withdrawing abraded material from within the housing (120, 218, 914); characterised in that the rotatable member (126, 920) has a substantially cylindrical outer abrasive surface for abrading stenotic material that penetrates the aperture (122, 220, 916) so that abraded material collects within the housing (120, 218, 914).
2. A catheter according to claim 1, wherein the rotatable member (126, 920) includes at least one groove (616, 716) extending generally along an outer surface of the rotatable member (126, 920) from its distal to proximal end, whereby abraded material may be withdrawn therethrough from a region distal the rotatable member (126, 920) to a region proximal the member (126, 920).
3. A catheter according to claim 1, wherein the housing (120, 218, 914) includes at least one groove (512) extending along an interior surface thereof from its distal to proximal end, whereby abraded material may be withdrawn from a region distal the housing (120, 218, 914) to a region proximal the housing (120, 218, 914).
4. A catheter according to claim 1, 2 or 3, wherein the rotatable member (126, 920) has an axial lumen (636, 658), thereby permitting passage of a guidewire therethrough.
5. A catheter according to claim 1, 2, 3 or 4, wherein the means (932-940) for withdrawing abraded material includes means (932, 934) for aspirating the interior of the housing (120, 218, 914) through an axial lumen (932) formed through the catheter body (110, 210, 910).
6. A catheter according to claim 5, wherein the means (932-940) for withdrawing abraded material further comprises a means (938, 936, 940) for flushing the interior of the housing (120, 218, 914).
7. A catheter according to any one of the preceding claims, further comprising an ultrasonic transducer (744) attached to the rotatable member (126, 920).
8. A catheter according to any one of the preceding claims, further comprising at least one inflatable balloon (224, 918) attached to the housing (920).

# Patentansprüche

1. Intravaskulärer Katheter zur Entfernung stenotischen Materials aus dem Gefäßsystem eines Patienten, welcher Katheter umfasst:
- einen länglichen Katheterkörper (110, 210, 910) mit einem proximalen (körpernahen) und einem distalen (körperfernen) Ende (114, 214, 112, 212);
- ein Gehäuse (120, 218, 914), das am distalen Ende (112, 212) des Katheterkörpers (110, 210, 910) befestigt ist, wobei das Gehäuse (120, 218, 914) ein hohles Inneres und eine hineinragende Öffnung (122, 220, 916) aufweist;
- ein rotierbares Element (126, 920), das sich im wesentlichen innerhalb des Gehäuses (120, 218, 914) befindet;
- eine Vorrichtung (924) zur Rotierung des rotierbaren Elements (126, 920); und
- eine Vorrichtung (932-940) innerhalb des Katheterkörpers (110, 210, 910) zur Entnahme von abgeriebenem Material aus dem Gehäuseinneren (120, 218, 914); dadurch gekennzeichnet, dass das rotierbare Element (126, 920) eine im wesentlichen zylindrische äußere Abriebsfläche zum Abreiben von stenotischem Material aufweist, das in die Öffnung (122, 220, 916) eindringt, so dass sich abgeriebenes Material innerhalb des Gehäuses (120, 218, 914) ansammelt.
2. Katheter nach Anspruch 1, wobei das rotierbare Element (126, 920) mindestens eine Furche (616, 716) umfasst, die sich generell entlang einer Außenseite des rotierbaren Elements (126, 920) von seinem distalen zum proximalen Ende erstreckt, wobei abgeriebenes Material durch sie hindurch von einer Region distal zum rotierbaren Element (126, 920) zu einer Region proximal zum Element (126, 920) entnommen werden kann.
3. Katheter nach Anspruch 1, wobei das Gehäuse (120, 218, 914) mindestens eine Furche (512) umfasst, die sich entlang einer Innenfläche davon von seinem distalen zum proximalen Ende erstreckt, wobei abgeriebenes Material von einer Region distal zum Gehäuse (120, 218, 914) zu einer Region proximal des Gehäuses (120, 218, 914) entnommen werden kann.
4. Katheter nach Anspruch 1, 2 oder 3, wobei das rotierbare Element (126, 920) ein axiales Lumen (636, 658) aufweist, durch welches der Durchgang

eines Führungsdrahtes ermöglicht wird.

5. Katheter nach Anspruch 1, 2, 3 oder 4, wobei die Vorrichtung (932-940) zur Entnahme von abgeriebenem Material eine Vorrichtung (932, 934) zum Absaugen des Inneren des Gehäuses (120, 218, 914) durch ein axiales Lumen (932) umfasst, das durch den Katheterkörper (110, 210, 910) verläuft.
6. Katheter nach Anspruch 5, wobei die Vorrichtung (932-940) zur Entnahme von abgeriebenem Material außerdem eine Vorrichtung (938, 936, 940) zum Spülen des Inneren des Gehäuses (120, 218, 914) umfasst.
7. Katheter nach einem der vorangehenden Ansprüche, außerdem umfassend einen Ultraschall-Transduktor (744), der am rotierbaren Element (126, 920) angebracht ist.
8. Katheter nach einem der vorangehenden Ansprüche, außerdem umfassend mindestens einen aufblasbaren Ballon (224, 918), der am Gehäuse (920) angebracht ist.

#### Revendications

1. Cathéter intravasculaire pour retirer un matériau sténosé du système vasculaire d'un patient, ledit cathéter comprenant :

un corps de cathéter allongé (110, 210, 910) comportant des extrémités proximale et distale (114, 214 ; 112, 212) ;  
un boîtier (120, 218, 914) fixé à l'extrémité distale (112, 212) du corps de cathéter (110, 210, 910), ledit boîtier (120, 218, 914) comportant un intérieur ouvert et une ouverture (122, 220, 916) à travers celui-ci ;  
un élément rotatif (126, 920) sensiblement à l'intérieur du boîtier (120, 218, 914) ;  
des moyens (924) pour faire tourner l'élément rotatif (126, 920) ; et  
des moyens (932 - 940) à l'intérieur du corps de cathéter (110, 210, 910) pour retirer le matériau abrasé de l'intérieur du boîtier (120, 218, 914) ; caractérisé en ce que l'élément rotatif (126, 920) comporte une surface abrasive extérieure sensiblement cylindrique pour abraser le matériau sténosé qui pénètre dans l'ouverture (122, 220, 916), de telle sorte que le matériau abrasé soit recueilli à l'intérieur du boîtier (120, 218, 914).

2. Cathéter selon la revendication 1, dans lequel l'élément rotatif (126, 920) comprend au moins une rainure (616, 716) s'étendant globalement le long

d'une surface extérieure de l'élément rotatif (126, 920) de son extrémité distale à son extrémité proximale, grâce à quoi le matériau abrasé peut être retiré à travers celui-ci d'une région distale de l'élément rotatif (126, 920) à une région proximale de l'élément (126, 920).

3. Cathéter selon la revendication 1, dans lequel le boîtier (120, 218, 914) comprend au moins une rainure (512) s'étendant le long d'une surface intérieure de celui-ci de son extrémité distale à son extrémité proximale, grâce à quoi le matériau abrasé peut être retiré d'une région distale du boîtier (120, 218, 914) à une région proximale du boîtier (120, 218, 914).

4. Cathéter selon la revendication 1, 2 ou 3, dans lequel l'élément rotatif (126, 920) comporte un conduit axial (636, 656), permettant ainsi le passage d'un fil de guidage à travers celui-ci.

5. Cathéter selon la revendication 1, 2, 3 ou 4, dans lequel les moyens (932 - 940) pour retirer le matériau abrasé comprennent des moyens (932, 934) pour aspirer l'intérieur du boîtier (120, 218, 914) à travers un conduit axial (932) formé à travers le corps de cathéter (110, 210, 910).

6. Cathéter selon la revendication 5, dans lequel les moyens (932 - 940) pour retirer le matériau abrasé comprennent de plus des moyens (938, 936, 940) pour rincer l'intérieur du boîtier (120, 218, 914).

7. Cathéter selon l'une quelconque des revendications précédentes, comprenant de plus un transducteur ultrasonore (744) fixé à l'élément rotatif (126, 920).

8. Cathéter selon l'une quelconque des revendications précédentes, comprenant de plus au moins un ballon gonflable (224, 918) fixé au boîtier (920).

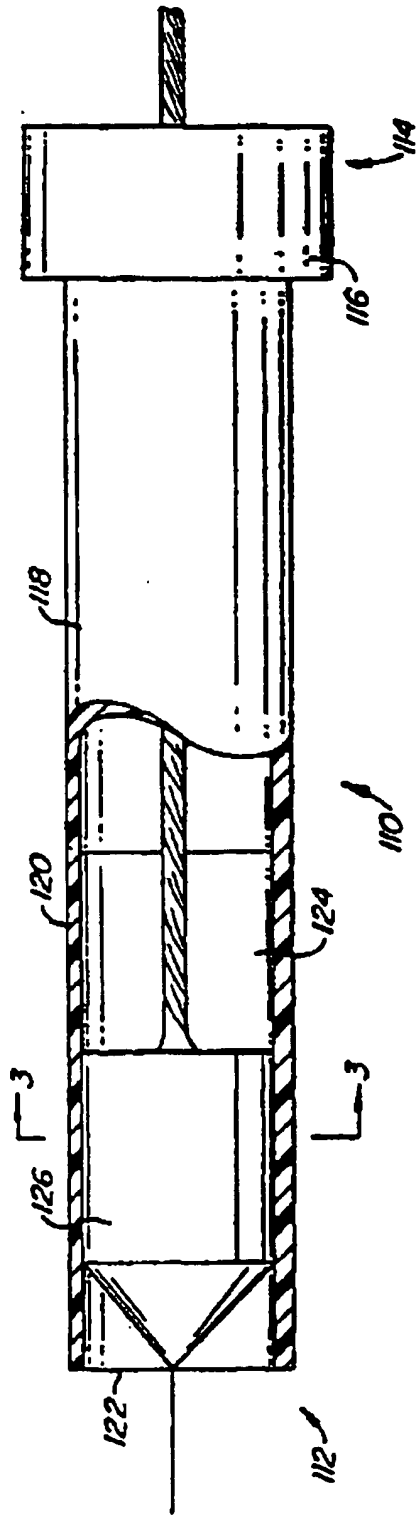


FIG. 1.

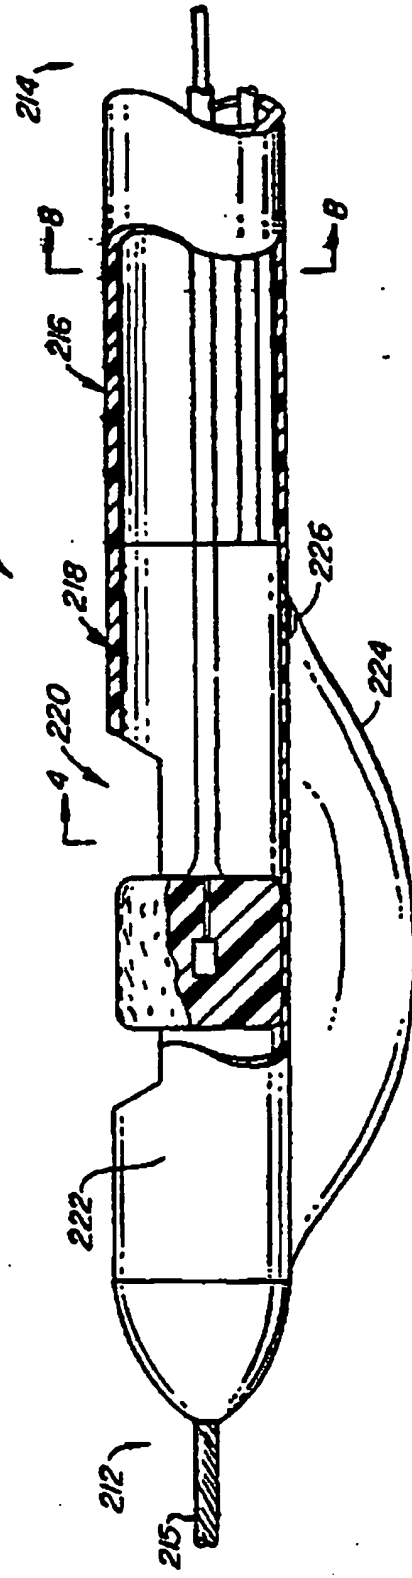


FIG. 2.

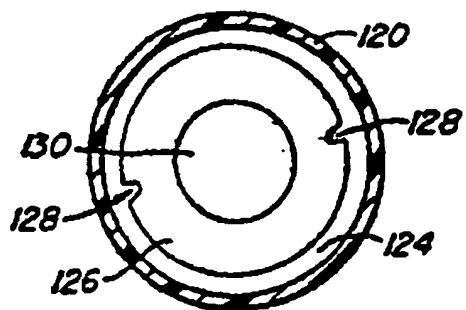


FIG. 3.

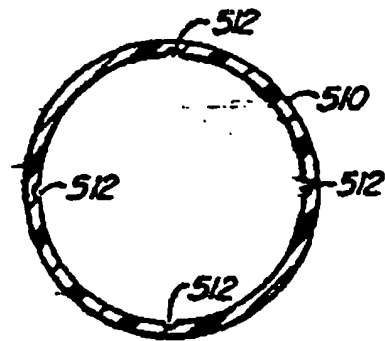


FIG. 5.

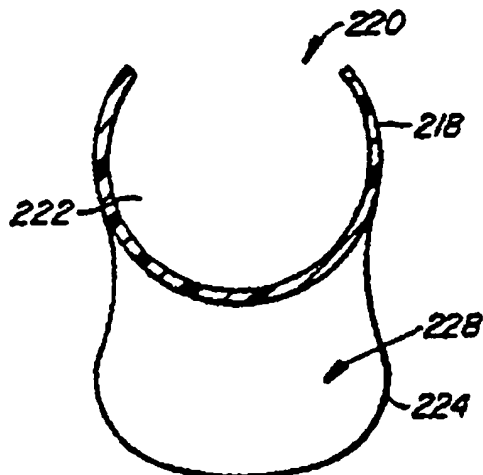


FIG. 4.

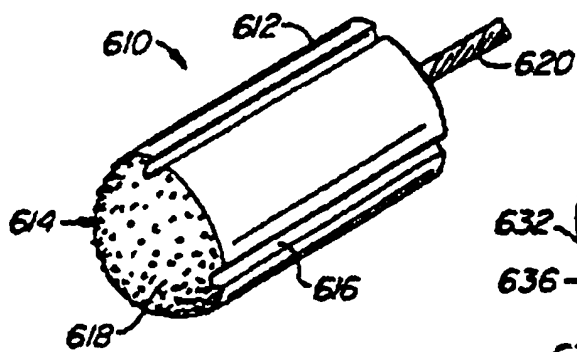


FIG. 6A.

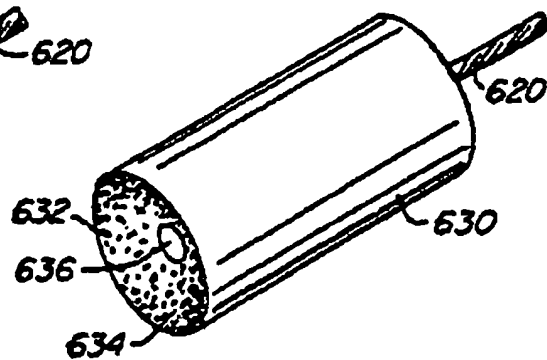
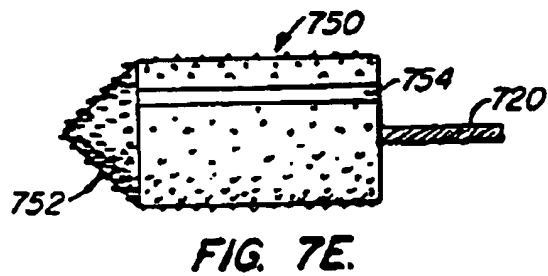
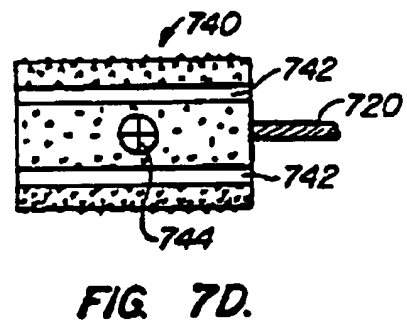
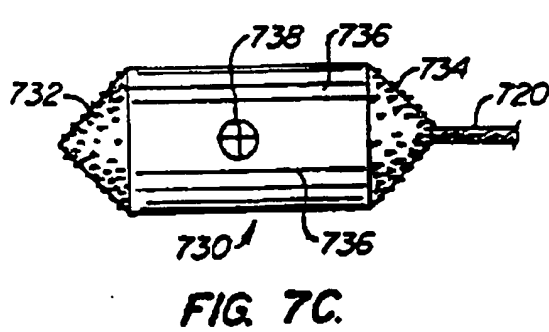
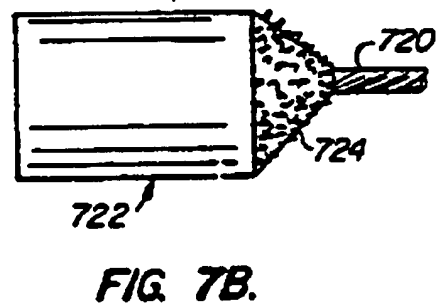
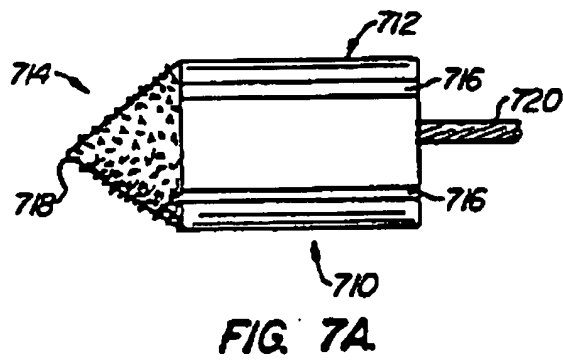
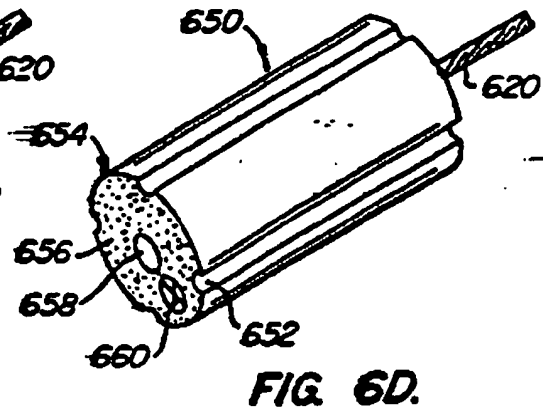
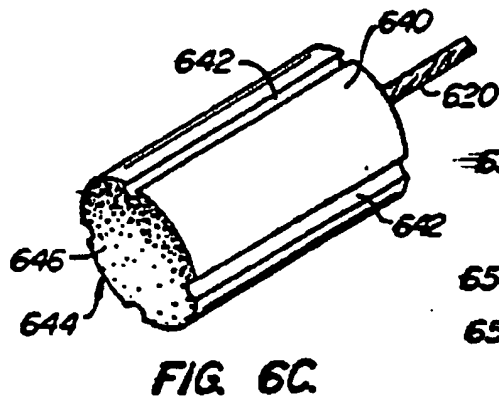


FIG. 6B.



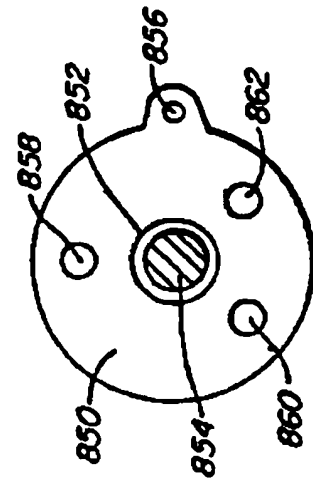


FIG. 8C.

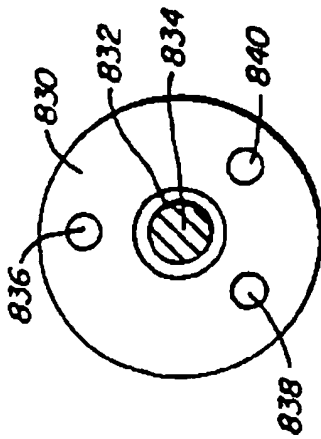


FIG. 8B.

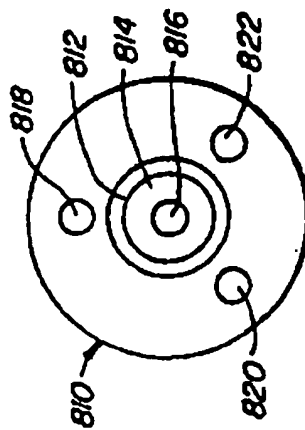


FIG. 8A.

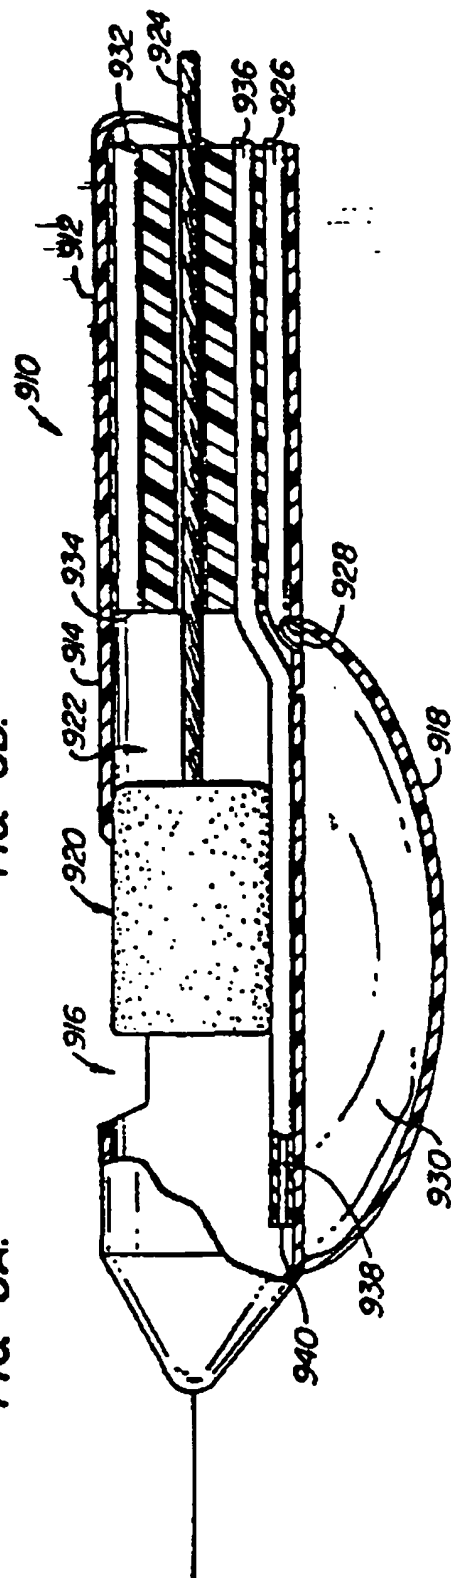


FIG. 9.